

This Page Is Inserted by IFW Operations
and is not a part of the Official Record

BEST AVAILABLE IMAGES



Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

**As rescanning documents *will not* correct images,
please do not report the images to the
Image Problem Mailbox.**

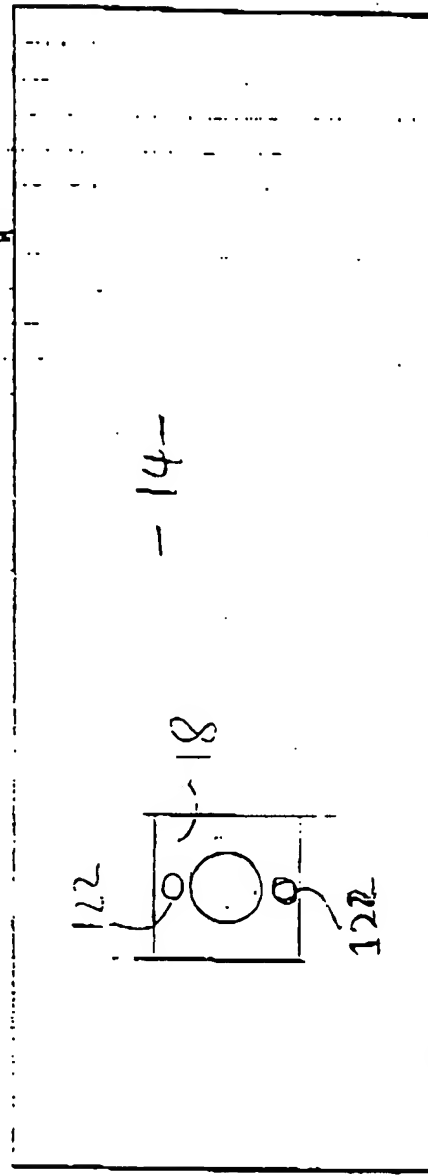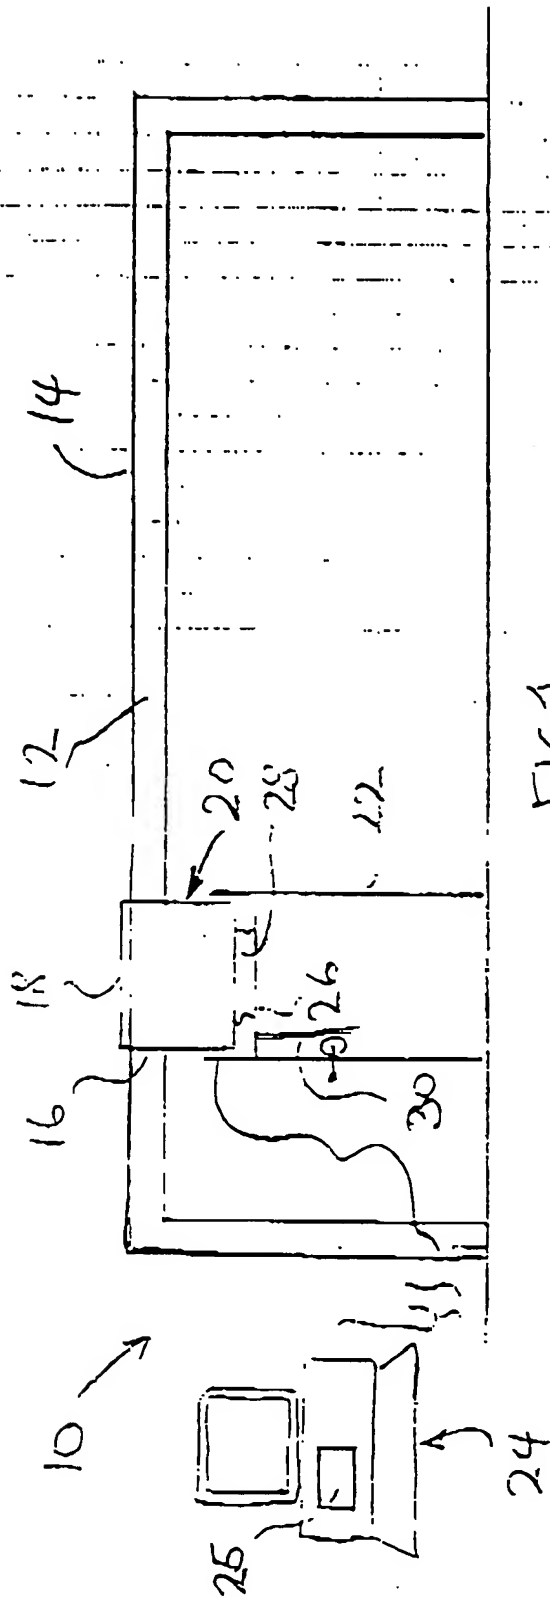

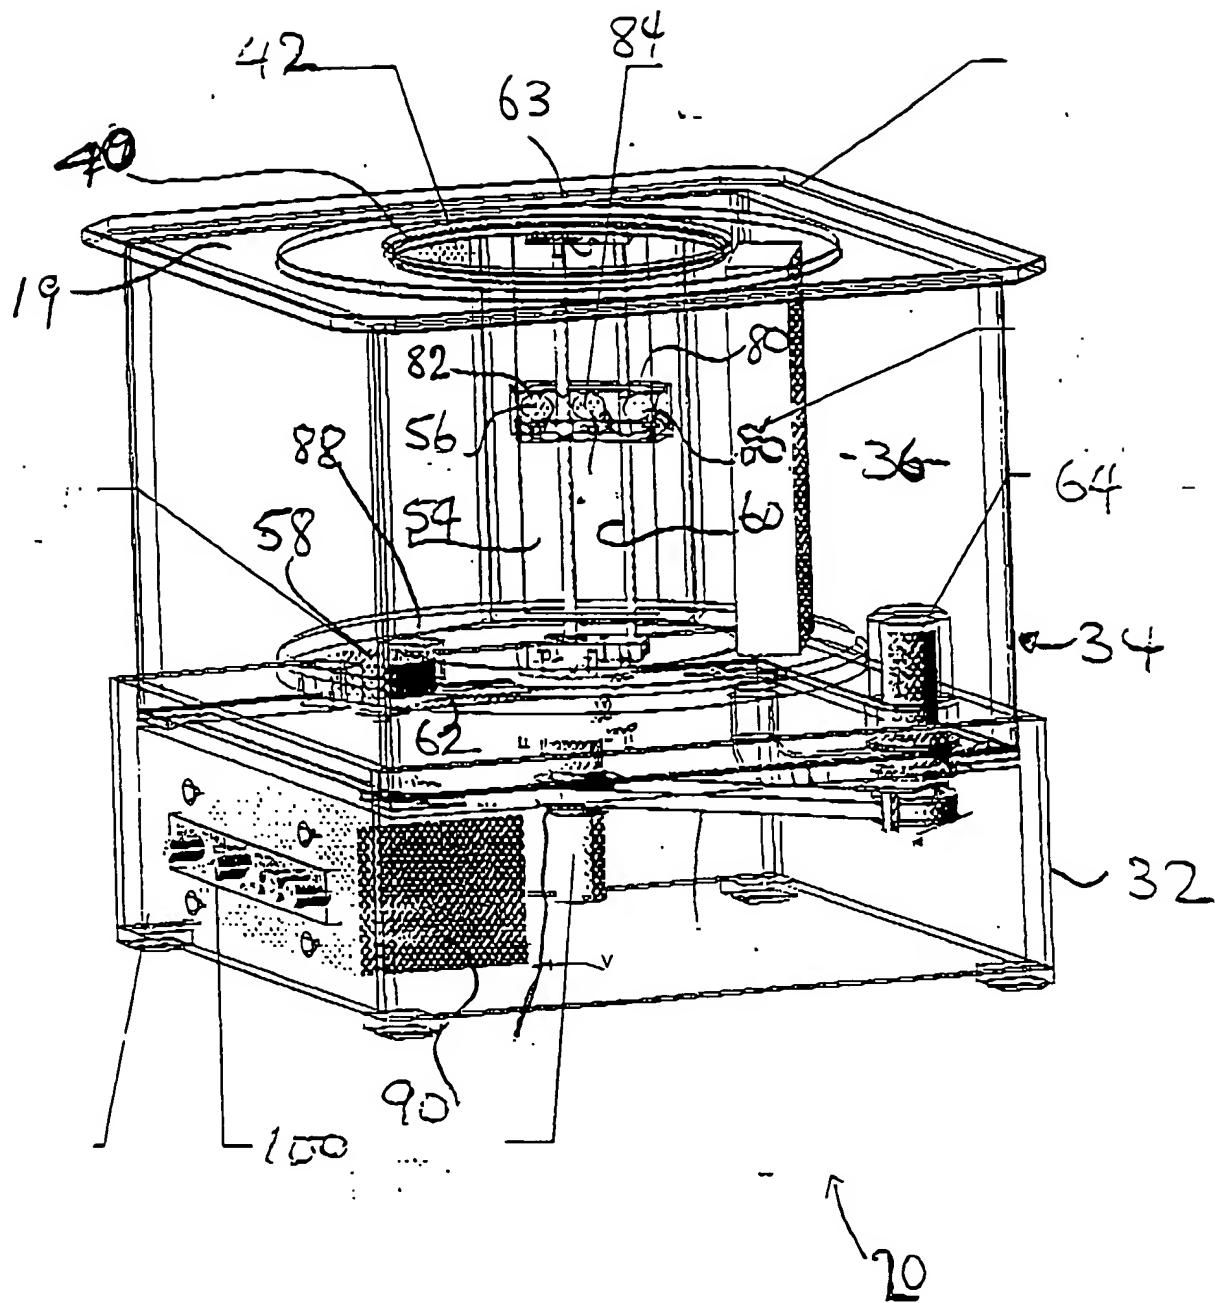


FIGURE 3

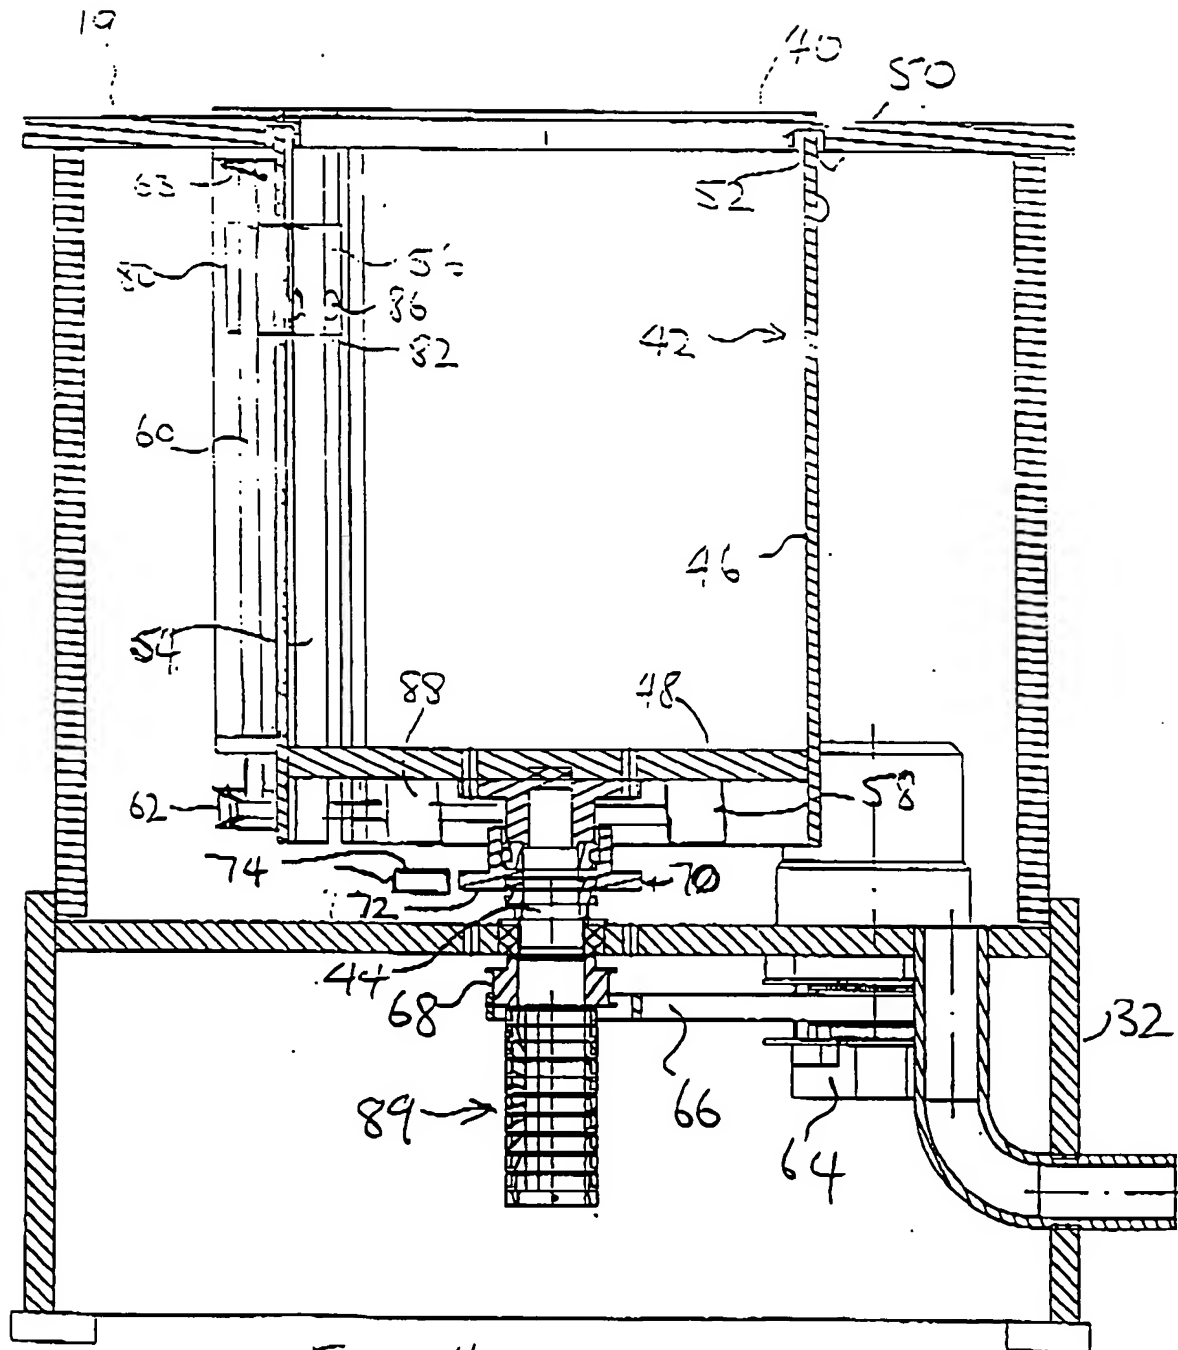
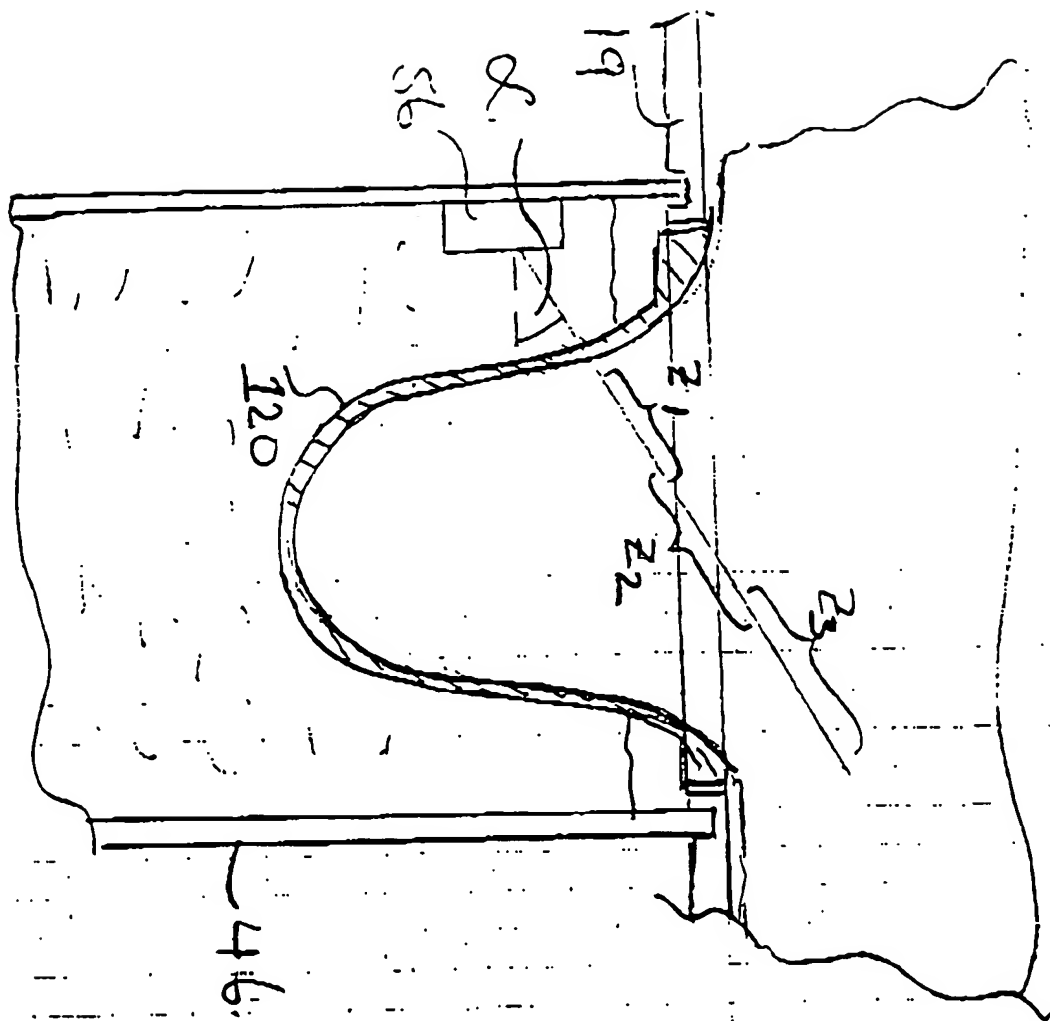


FIG. 4



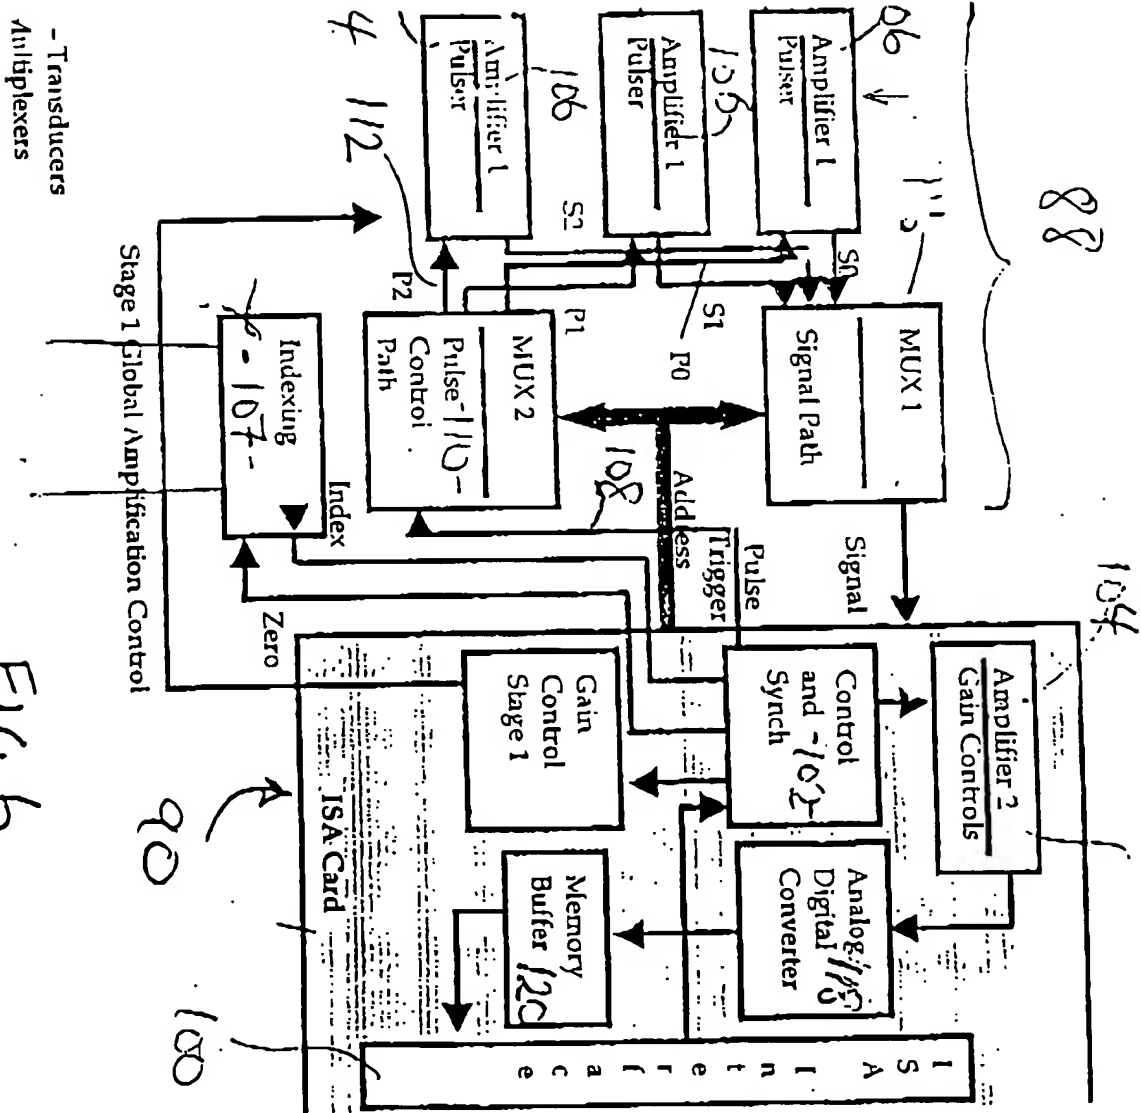


Fig. 6

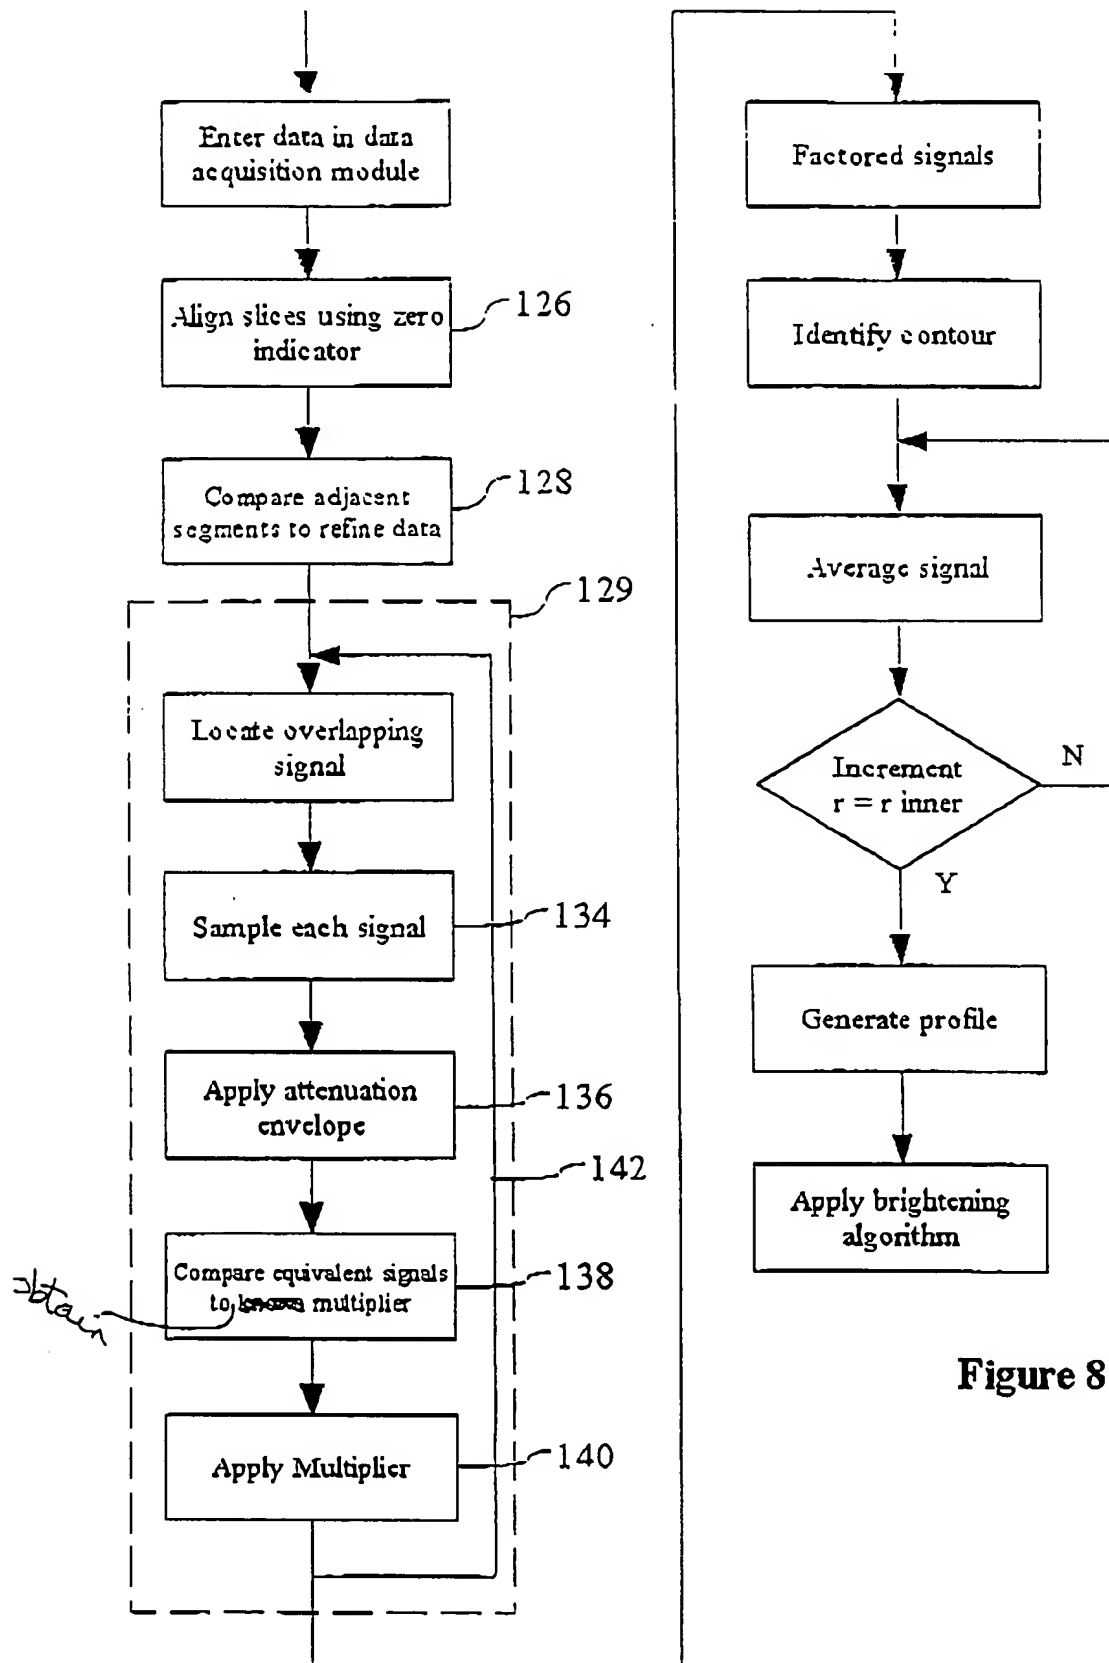


Figure 8

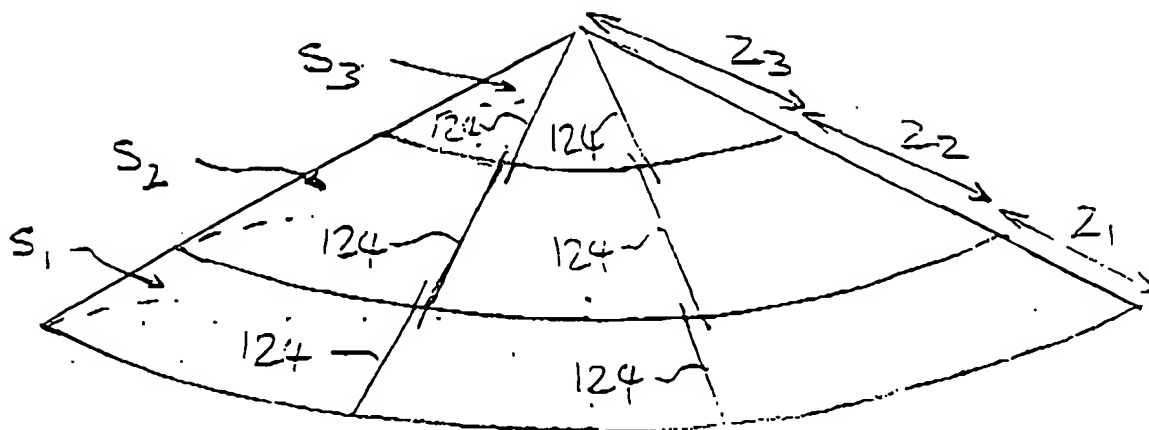


FIG 7

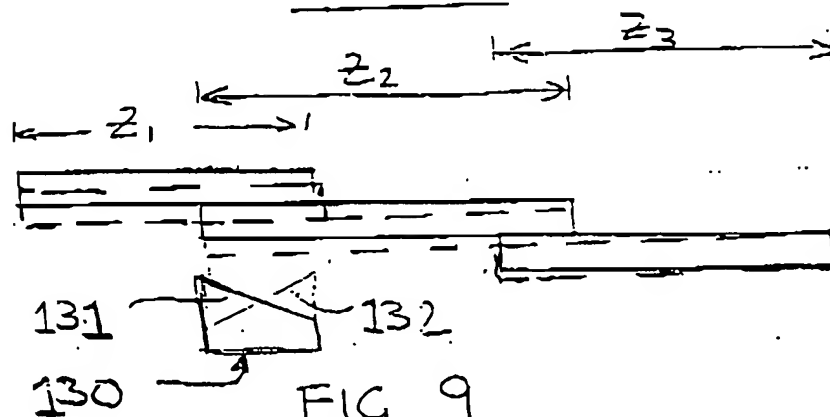


FIG 9

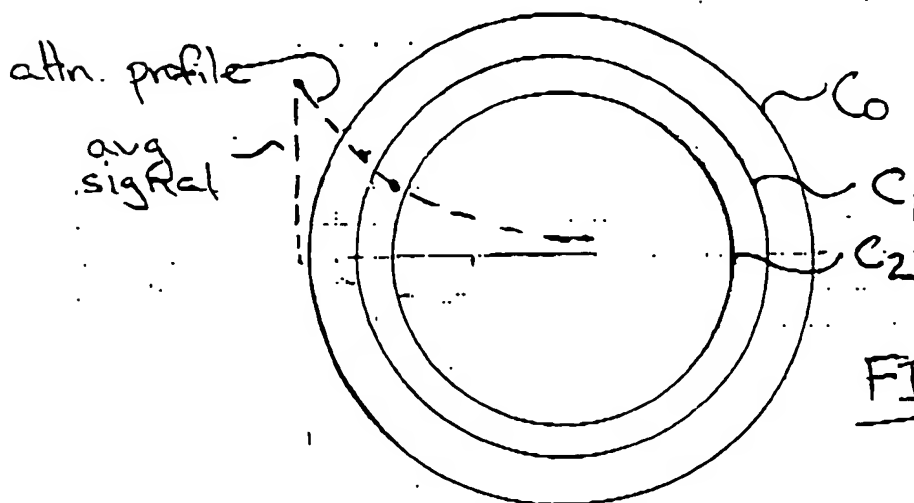


FIG 10.

FIGURE 11

The Medipattern Corporation - Connected to MED

medipattern

Registration Cabinet Scan MPR Logout

Acq. Params: **Recon 3.4mm** **Serial 9** **Serial 13**

USG USG Scanner 5

Device Settings

Step Size (0.1mm): 10
Vertical Count: 110
Vertical Start (0.1mm): 0

Card Settings

Amplifier: 1 V/V
Sampling: 20 MHz
Breast: Right

Preview/Scan Mode: Quality Size: SizeB

Transducer Preamp

17 25 312

POWER

On Off GoTop

VERTICAL MOTOR

<< UP DN >>

Cine Controls

Cine Type: YoYo Loop
Speed (0.5): 6
Play Stop


Preview Scan RECON 4:1:14 4:1:14

Dev Debug

Acquisition

Acquisition: **Recon 3.4mm**

Folder ID: 1010 Name:

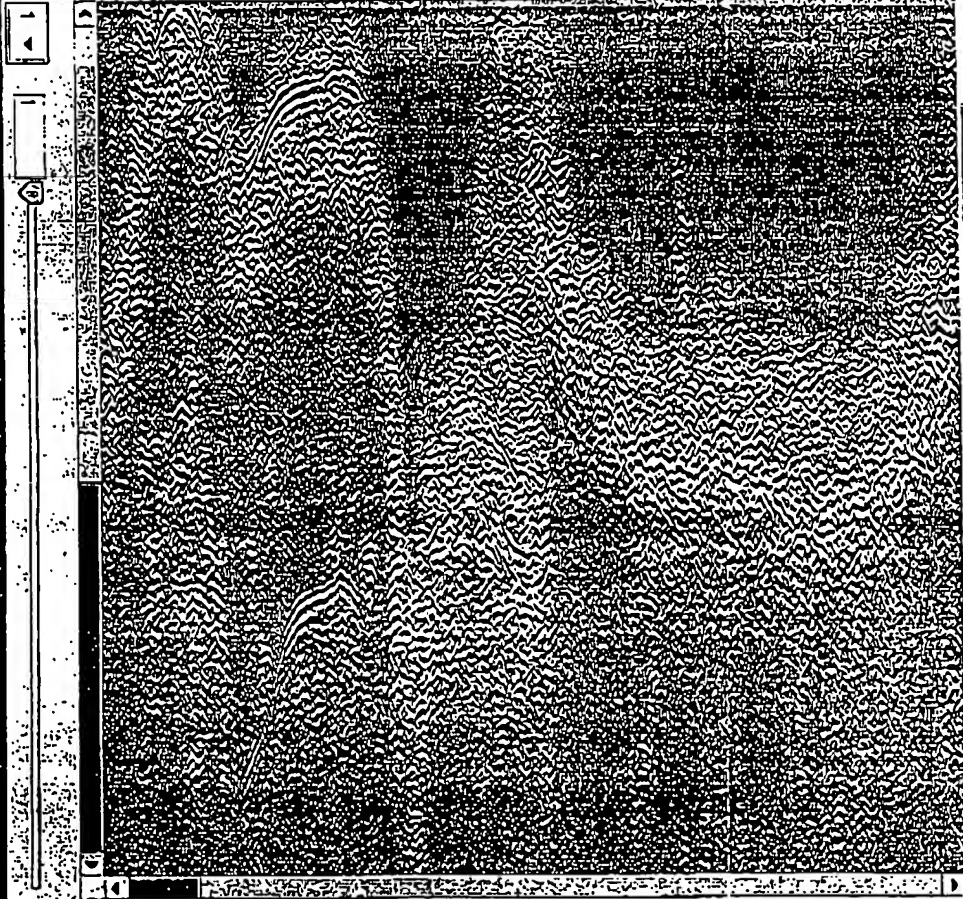

1 0 1 2 3 4 5 6 7 8 9 10 11 12 13 14 15 16 17 18 19 20 21 22 23 24 25 26 27 28 29 30 31 32 33 34 35 36 37 38 39 40 41 42 43 44 45 46 47 48 49 50 51 52 53 54 55 56 57 58 59 60 61 62 63 64 65 66 67 68 69 70 71 72 73 74 75 76 77 78 79 80 81 82 83 84 85 86 87 88 89 90 91 92 93 94 95 96 97 98 99 100